

**Fig. 1**

(Prior Art)

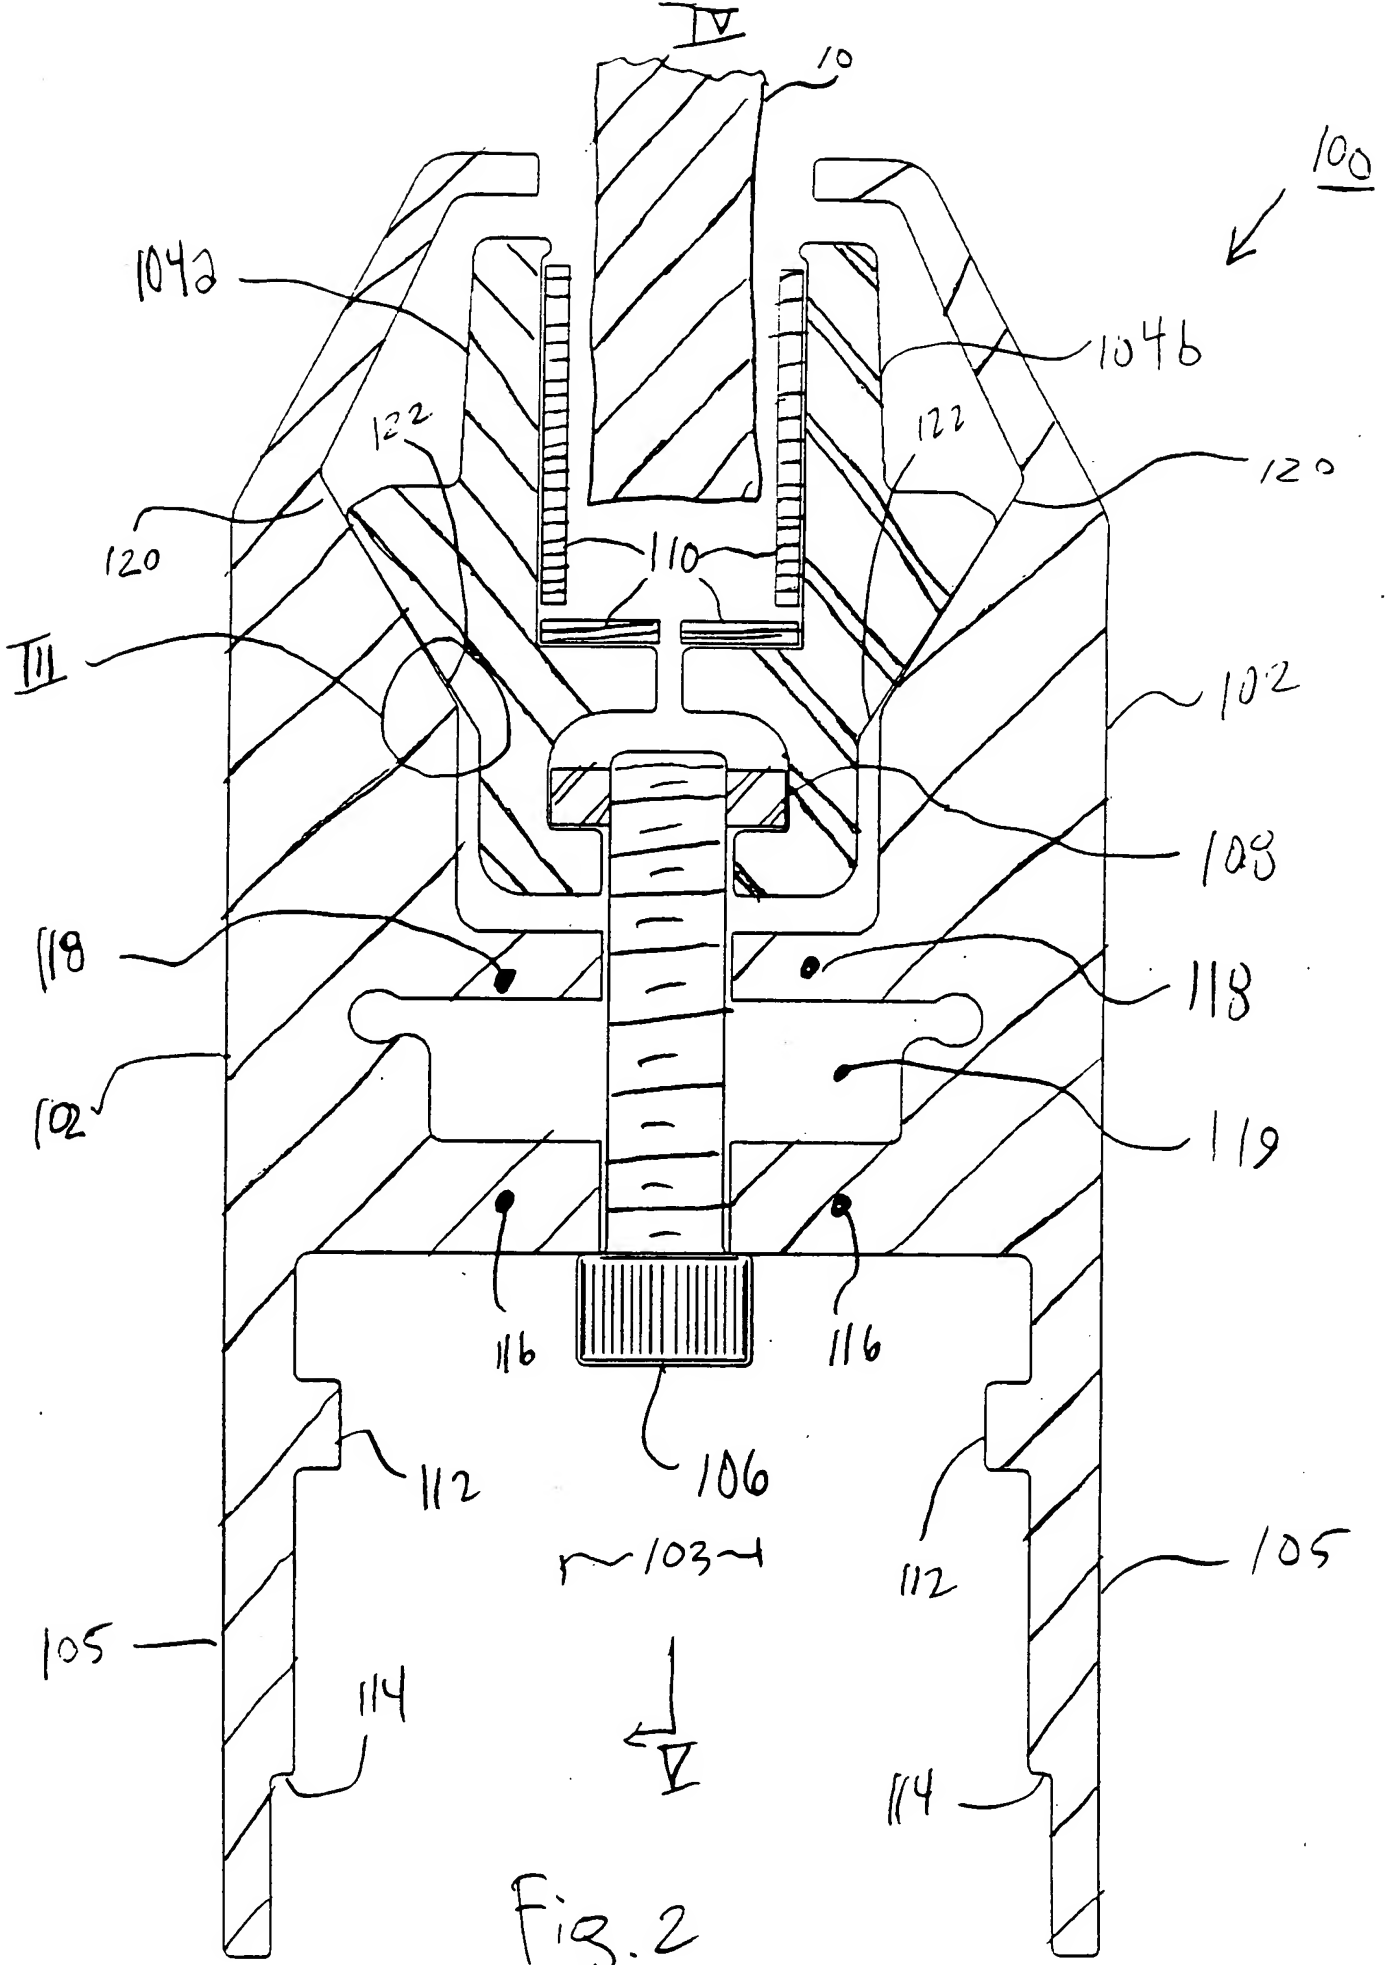


Fig. 2

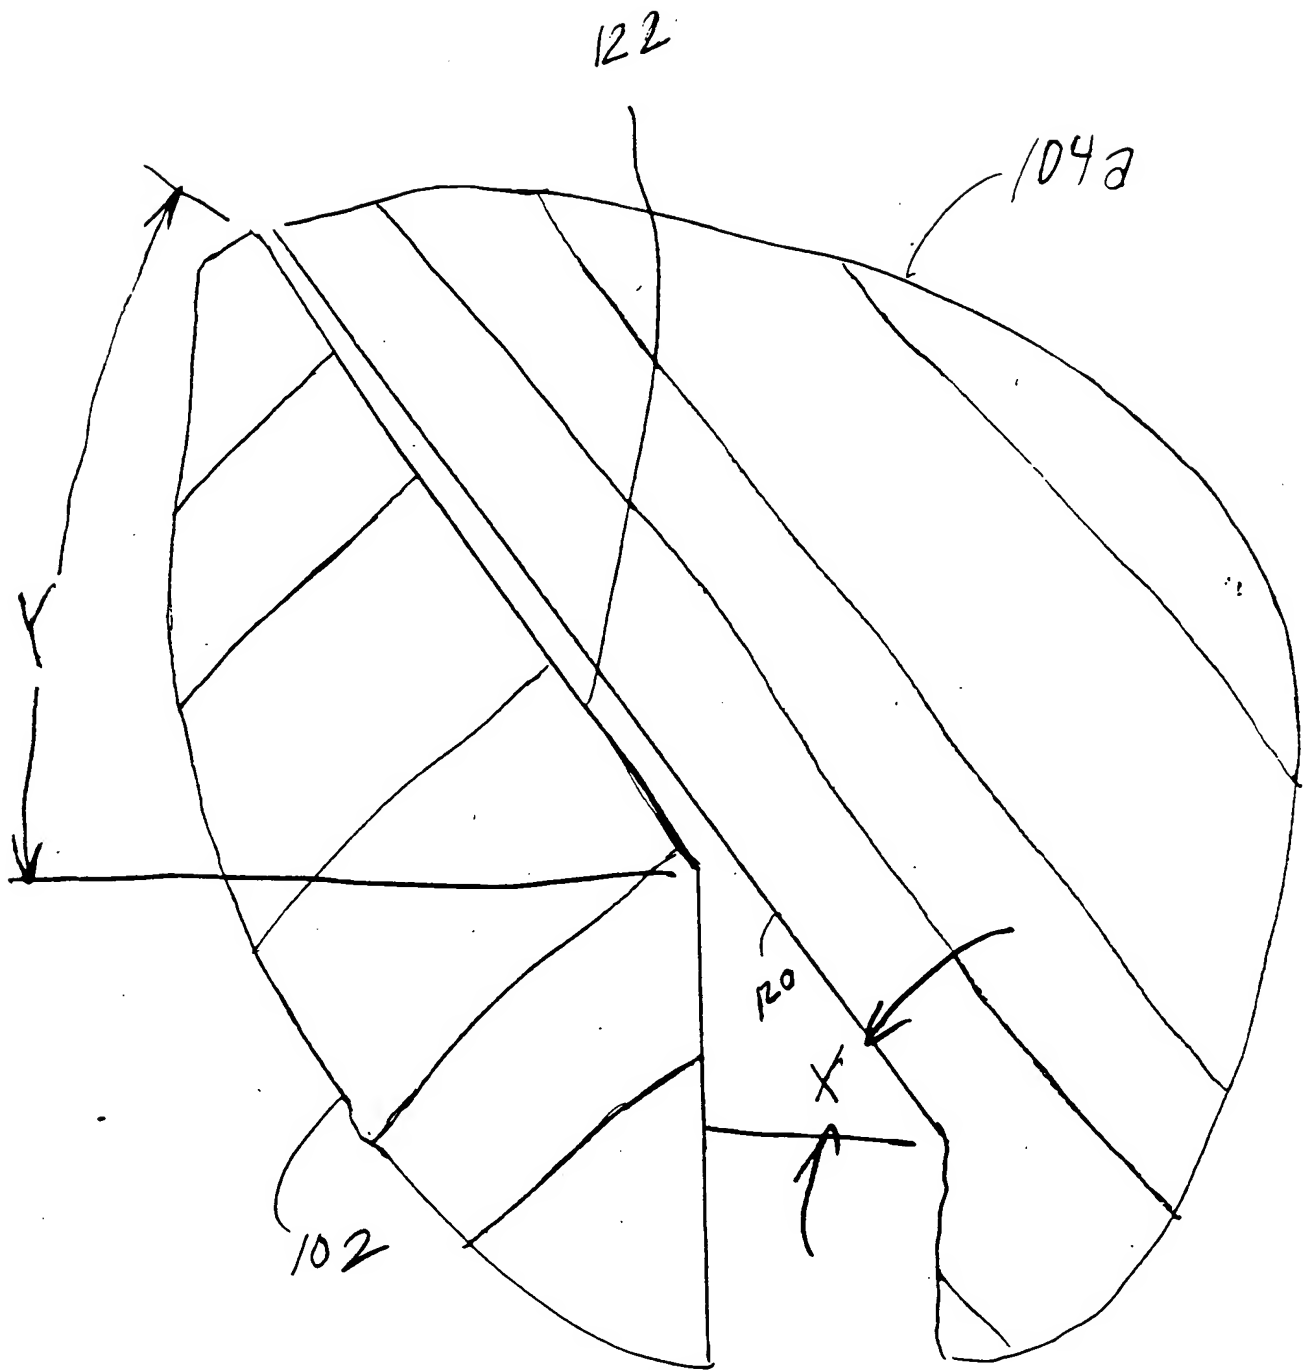


Fig. 3

Fig. 6

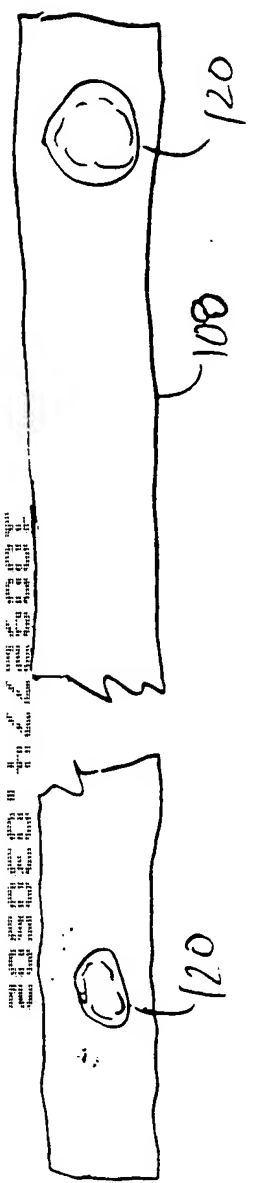


Fig. 4

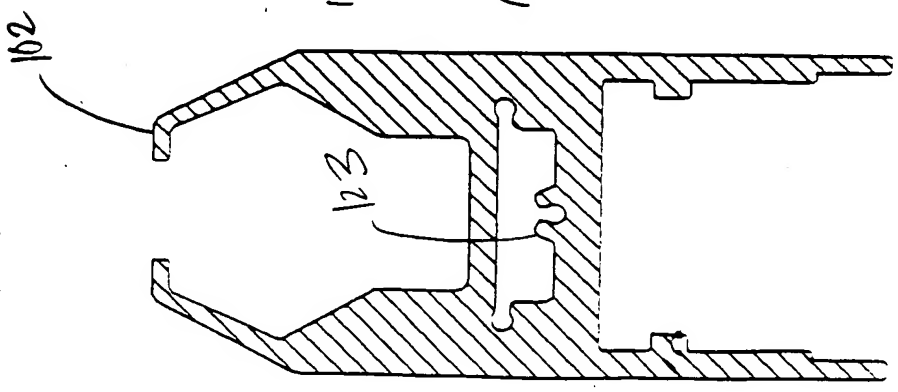


Fig. 5


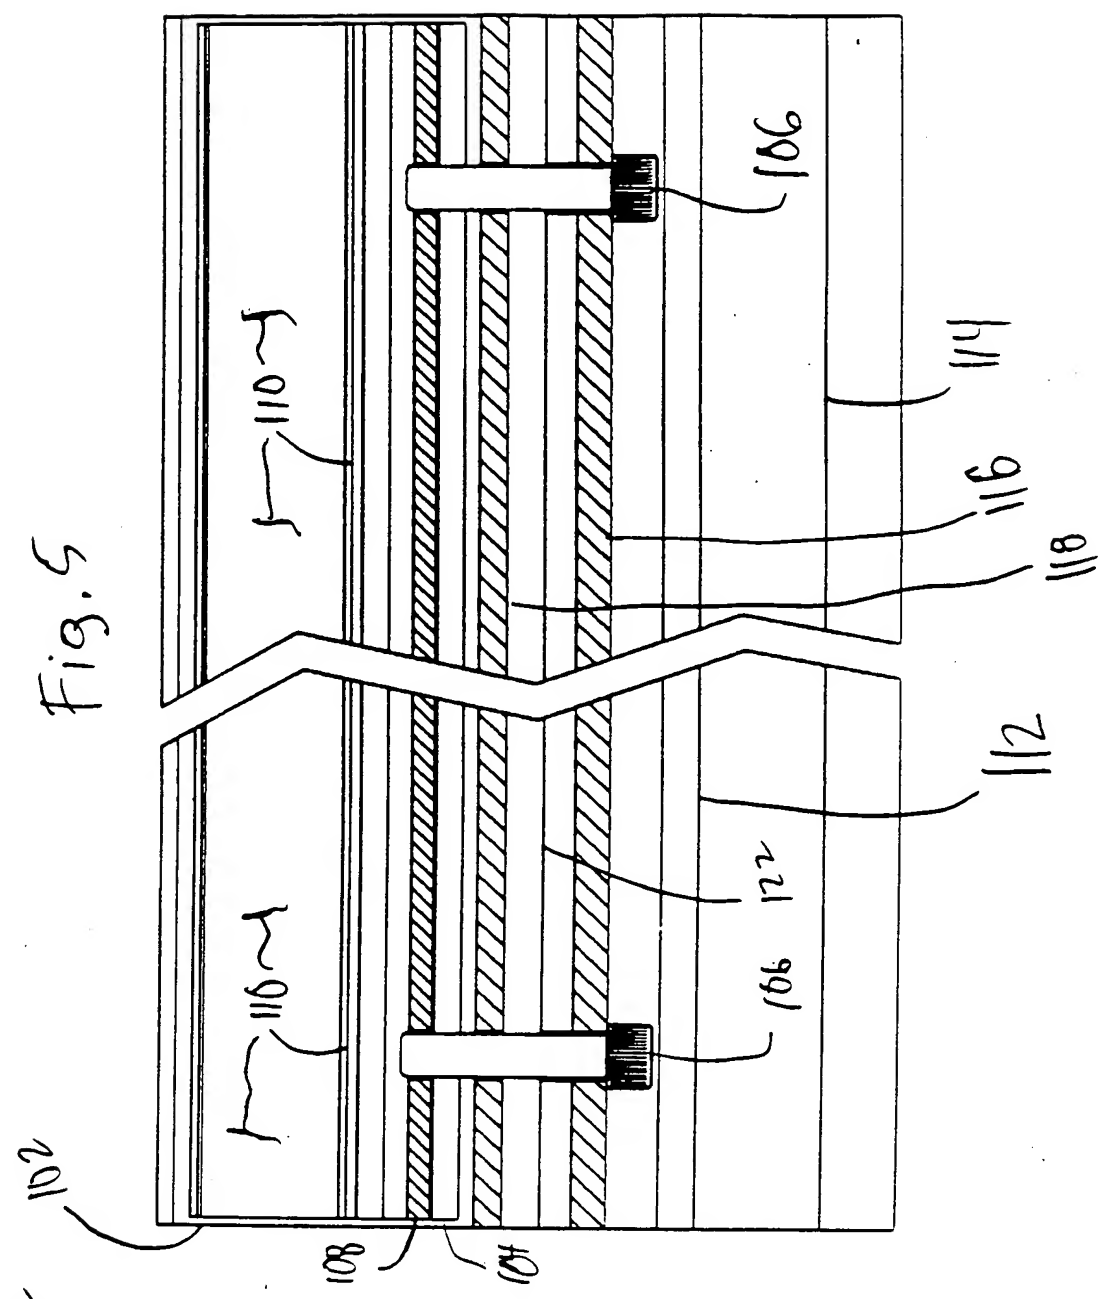




Fig. 7

XI  
↓

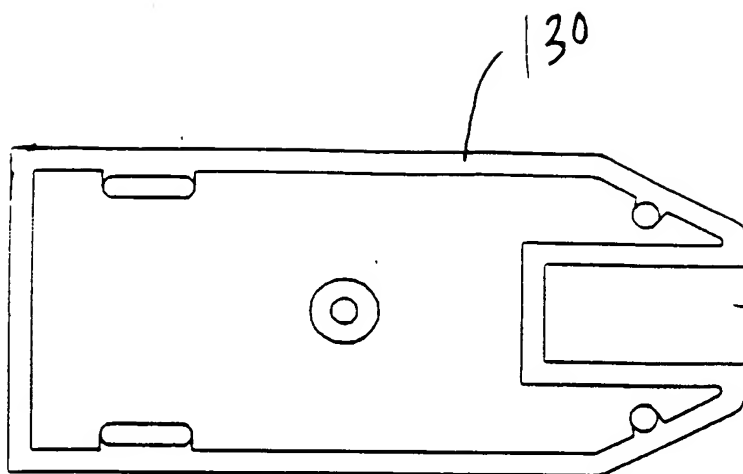

XI  
↓

Fig. 8

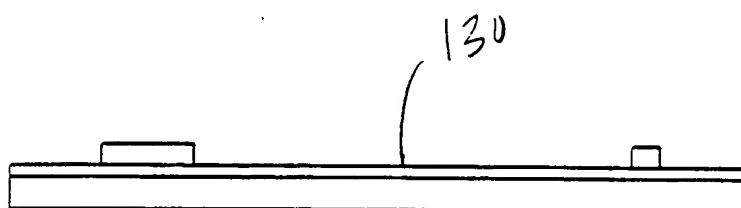


Fig. 9

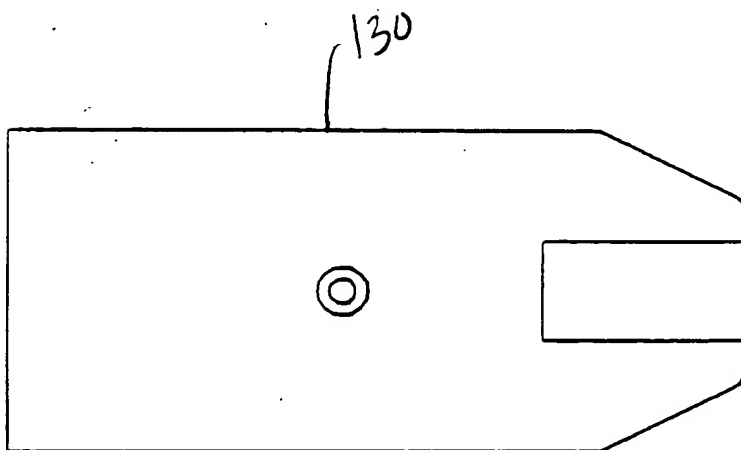


Fig. 10

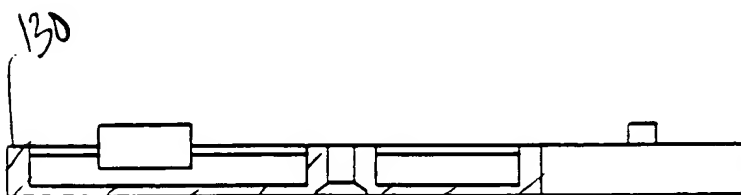


Fig. 11

FIG. 12 is a cross-sectional view of the device 100 taken along line A-A of FIG. 11.

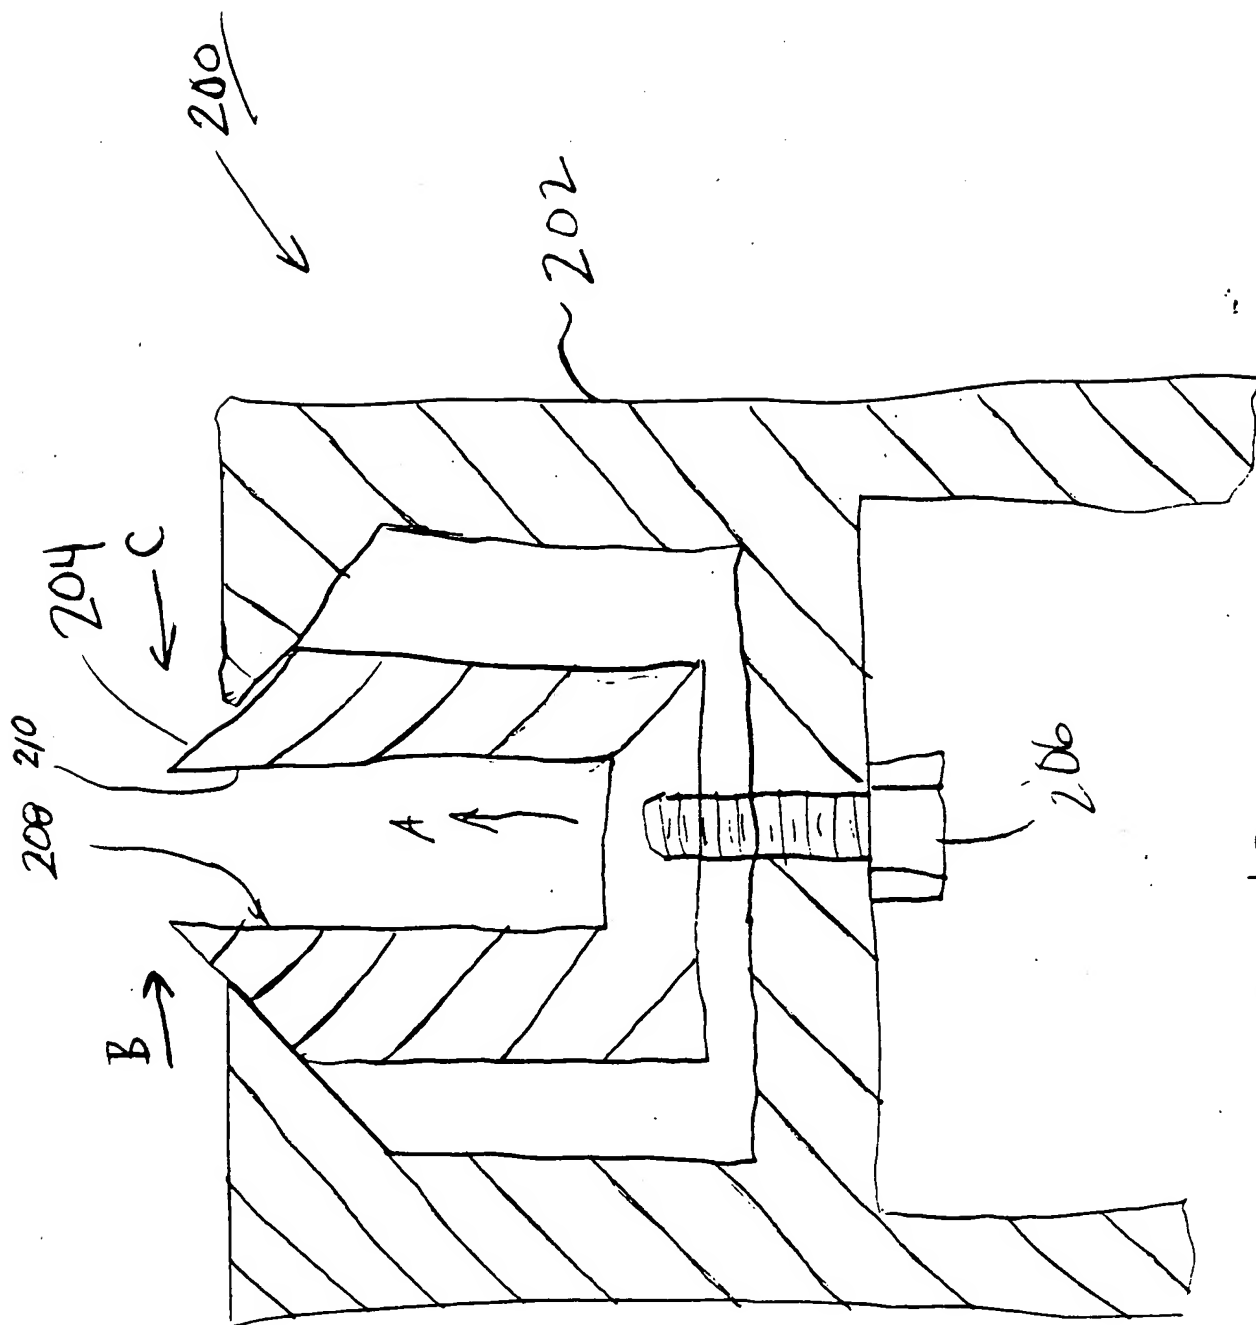


Fig. 12

